

Model YR417

Manual Microtome

Instruction Manual

Thank you very much for purchasing our Model YR417 Manual Microtome.

Please read the “Operating Instructions” and “Warranty” before operating this unit to assure proper operation. After reading these documents, be sure to store them securely together with the “Warranty” at a hand place for future reference.



Warning: Before operating the unit, be sure to read carefully and fully understand important warnings in the operating instructions.



OUR SERVICES

Benefits and Support

In Kalstein France, we take care of the full satisfaction of our customers, that is why we provide value-added services of the highest level based on our experience.



Online Inductions and Trainings

In any part of the world, receive your induction or training from our specialized team of engineers



Quick Response

Our work team is always available to response all your consults or questions, in order to support you in any situation.



#Letsgivemore

Thanks to your purchase, a donation will be made to a non-profit foundation that fights against breast cancer and helps most vulnerable communities.



Technical Support

Enjoy of personalized advice for the correct preventive and corrective maintenance of your equipment, thanks to Kalstein's manuals and articles, special catalogues and video tutorials.



Delivery Logistics

We take care of all the necessary logistics for the dispatch of your goods, whether is by sea, land or air.



Kalstein Worldwide

With more than 25 years growing with our customers, Kalstein's multiformat and modern content, is now present in more than 10 countries and increasing.



1. Important Notes

The scientific knowledge and the up-to-date technology we master have been displayed by the information, data, precautions, and the parameters of adjustment provided in this manual through our investigation in the field.

With the rapid development of technology, we are not responsible for providing the renewed manuals or any copy of them to the customers.

We will not shoulder the responsibilities for the results caused by the instructions, drawings, and technological requirements in this manual in case they conflict with the laws in the country of the customers, especially we are not responsible for any damage and other bad results caused by abusing instructions of this manual.

The instructions, drawings and technological requirements and other information in the manual should not be taken as the guarantee for the performance of the product. Only those items stipulated in the contract have the legal effect.

We own the right to alter the technological parameters and the processing crafts, and we have no obligation to notify the users about them.

The copyright of this manual belongs to Kalstein France, and it is under the protection of laws. Wholly or partly copy of the script and the photos or drawings by printing, photocopying, microfilming, electronically copying and other ways are not allowed except under the written permission of our Company.

The serial number and date of production are attached on the nameplate at the back of the instrument.



2. Contents

1、 Important Notes.....	1
2、 Contents	2
3、 Handwheel operation	3
4、 Technical parameters.....	5
5、 Brief introduction	5
5.1 Sketch of YR417 Microtome.....	5
5.2 Description.....	6
6、 Unpacking and installation	6
6.1 Unpacking	6
6.2 Requirements for handle	6
6.3 Trimming	6
7、 Installation.....	7
7.1 Installation of specimen clamp	7
7.2 Installation of accessories	8
7.3 Installation of Blade Holder and its Base.....	8
7.1 Installation of Waste Tray.....	7
8、 Ways of operation.....	9
8.1 Section Thickness.....	9
8.2 Handwheel	9
8.3 Trimming.....	10
8.4 Sectioning	10
8.5 Retraction	11
9、 Regular Operation	11
10、 Errors Checking and Solutions.....	12
11、 Cleaning	13
12、 Maintenance	13
13. Appendix.....	15

3. Handwheel operation


Safety Device

Attention: Lock the Handwheel before cleaning!

Quick locking lever for Handwheel

Attention: Remember to lock the handwheel and cover the blade with the protection fitting before operating the blade or specimen and changing the blade and specimen.

The handwheel can be locked at any position with the locking handle (1) at right side of the pedestal of the microtome. The two positions (Up=lock; Down=loosen) of the locking handle are marked at the pedestal of the microtome.

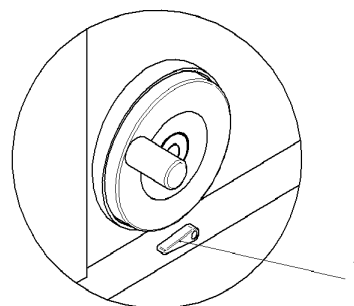

Ways of operations:

- Pull the locking lever (1) to “Up” to mechanically lock the handwheel, the handwheel cannot be turned.
- Pull the locking lever (1) to “Down” to lose the handwheel, and the handwheel can be turned around.

Blade-protecting lever on the blade holder

Attention: Remember to lock the handwheel and cover the blade with the protection lever before operating the blade or specimen or changing the specimen and during the break.

There is protecting lever on each blade holder, with which the blade edge can be wholly covered.

Transport and Install


- Pay attention to “Technical Parameters” in Chapter 4.
- The instrument can only be erectly placed in the course of transportation.
- Avoid grasping the handles of the wheel and the handwheel or the knob for adjusting the slice thickness in the course of moving the instrument.
- It is not allowed to remove or change the protecting devices equipped on the instrument and its appurtenance.

Operation

- Be very careful when using the blades and disposable blades. The sharp edge may cause serious injury by misoperation.
- No blade or the blade-holder with blade is allowed to be randomly placed. The blades should always be kept in blade cases except for use.
 - The blade is not allowed to be placed with its edge upward.
 - No catching a falling blade with hands at any time.
 - Firmly clamp the specimen before installing the blade.
 - Remember to lock the handwheel and cover the blade with the protection fitting before operating the blade or specimen or changing the specimen and during the break.
- No liquid is allowed to flow into the instrument.
- There is an alarm function when the handwheel is rotated to the top. but remember to keep the handwheel backward!

Cleaning

- Lock the handwheel before cleaning the instrument.

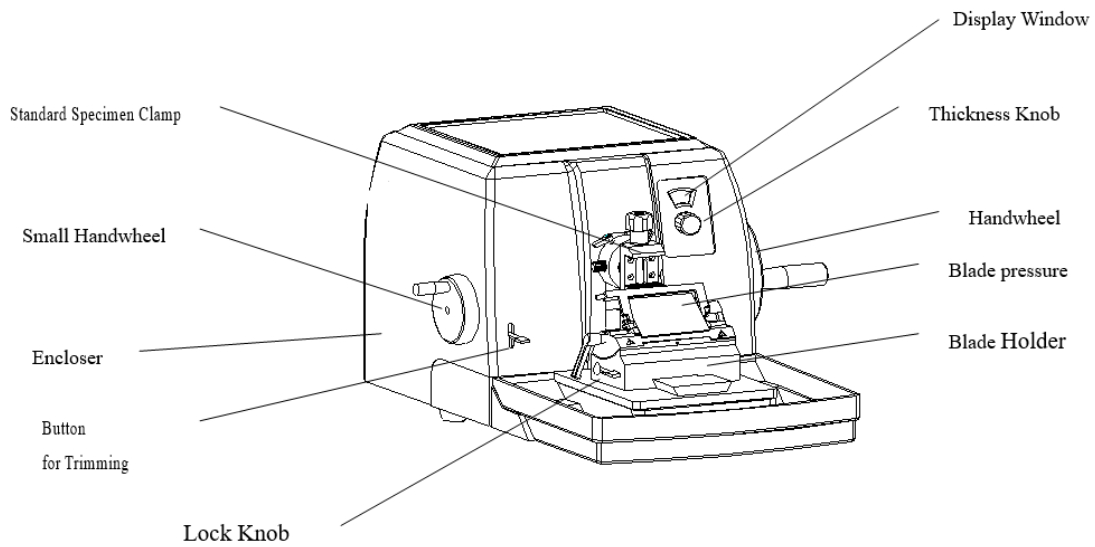

5.2 Description

Model YR417 is a manually operated microtome by wheel-turning. The guiding-lines for the vertical and horizontal movement of the specimens are seamless and free from maintenance. Specimen is fed by the turning the handwheel. And all the parts of the instrument are covered into the encloser. The handwheel can be smoothly turned for slice cutting. Selection of the slice thickness can be adjusted by a knob.

6. Unpacking and installation

6.1 Unpacking

- Unpack the wooded crate to take out all Appurtenances and the Instruction.
- Hold the base of instrument and take it out.

Attention: Avoid grasping the handle of the handwheel and the wheel, or the knob for adjusting the slice thickness in the course of moving of the instrument.

Instrument setting

- The instrument should be set on the stable platform in the lab.


6.2 Requirements for Handle

- Stable and no vibration for experimental platform
- No vibration on the floor.
- Leave enough room for the convenient operation of the handwheel and the wheel.

7. Installation

7.1 Installation of Specimen clamp


The adjusted setting of specimen clamp has been installed onto the

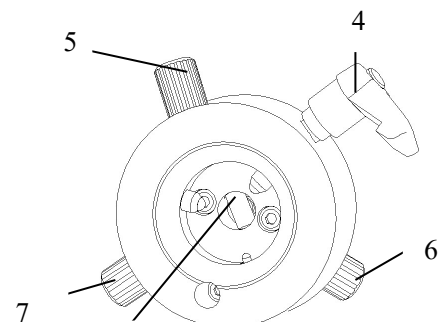

mainframe. But as the ordered component, the setting hasn't preinstalled and adjusted, it needs installation and adjustment.

Standard specimen clamp

- Lock the handwheel
- There is a coattail holder-leading on the standard specimen clamp (1), loosen the clamp handle (4), insert the coattail holder-leading into the coattail slot (3), when completing, lock up the handle (4) .

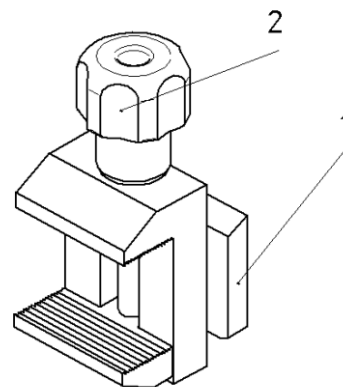

- Turn downward the locking handle to loosen it (7), the position of the specimen clamp can be adjusted through the screw (5) and (6) .

Attention: The screw (5) and (6) should be adjusted simultaneously within their range of turning.]


- The screw (5) for Up / Down, and screw (6) for Right / Left. In the course of adjustment, the locking handle (7) should be loosened.

- Once the position of the specimen clamp fixed on, turn upward the locking handle (7) to lock it down. .

- Change the specimen clamp: Loosen the locking handle (4) to take out the specimen clamp from the coattail slot for a new one.

Universal Cassette Clamp


- Lock up the handwheel
- The way for installation and adjustment is the same
- The general specimen case clamp can horizontally or vertically specimen cases commercially acquired.

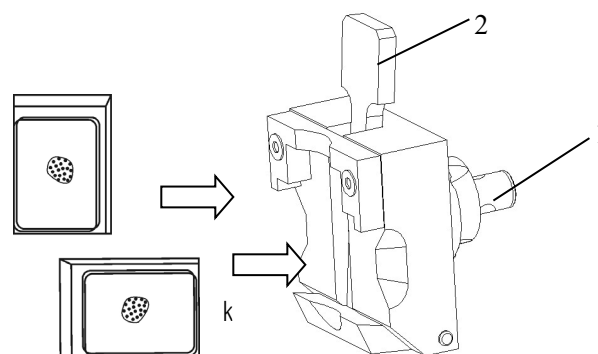

- Pulling forward the Board Pole (2) .
- Horizontally or vertically put in the specimen case.
- Loosen the Board Pole (2) to clamp the specimen case.

7.2 Installation of Accessories

Attention: please don't insert the disposable blade before the Blade holder is securely and properly installed on the Microtome! The disposable blade shall be taken out before dismantling the blade holder for safety concern.

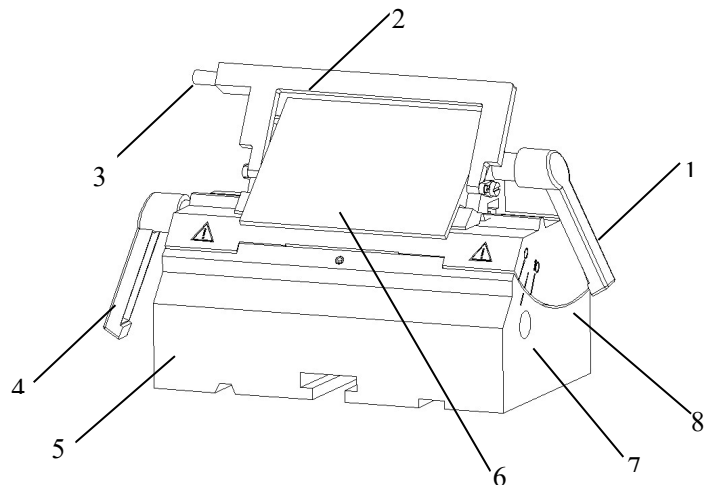

7.3 Installation of Blade Holder and its

Base

- Move the blade holder base (5) forward and backward, and counterclockwise turn the clamping lever (1).
- Install it on the T-block on the base of the Microtome, and clockwise turn the clamping lever (1).
- Loosen the screw (7), turn the copper threaded sleeve in the middle and the clamping positions of the lever could be adjusted.
- The appropriate clamping angle for the blade holder shall be approximately $8\sim 10^\circ$ for cutting.
- The screw (7) could be loosened before adjusting the cutting angle

Loose the locking lever (4) and move the pressure board (6) left or right to move the disposable blade to any position.

The blade holder can be used for the low-profile disposable blades.

- Turn and loosen the locking lever (1), and insert the blade into the groove edgewise, and turn the locking lever (4) after putting into proper place and make the blade clamp (3) to fix the blade at its position
- The knife guard on disposable knife holder consists of a red adjustable handle (2). To cover the cutting edge, fold the knife guard handle (2) upwards as illustrated in Fig
- When changing the disposable blade, fold the knife guard handle upwards, loosen the locking lever (1), push the strip (3) inside and the blade will be push out.

Attention: Remember to lock the handwheel and cover the blade with the protection fitting before changing the specimen and during the break of operations.

7.4 Installation of Waste Tray

Push waste tray paralleled to bottom of base of machine until the end.

8. Ways of Operation

8.1 Section Thickness

Section thickness range can be done by adjusting the knob located on the right upside of the front part of the microtome.

Each grade of the selection of the slice thickness can be efficiently positioned (1)

- Section Thickness Range: 0—60 μ m


- Setting value:

 - 0—20 μ m Increment 1 μ m

 - 20—60 μ m Increment 5 μ m

- Display Window (2) shows Section

Thickness range

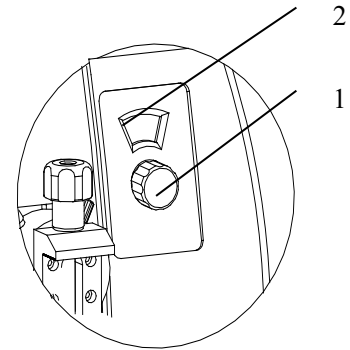

8.2 Small Handwheel

The provision can be quickly done by the handwheel located on the side of the instrument.

Turn the handwheel clockwise to make the specimen move to direction for making section

The handwheel is designed to make the specimen horizontally quick move to or departure from the slice cutting. When the handwheel move to the forward and backward utmost position, it will become heavier, but when the handwheel move to the forward utmost position, no specimen will be provided.

Attention: Be careful enough to ensure the specimen is on the specimen clamp. Damage will be done to the blade if the blade meets the metal specimen clamp.

8.3 Trimming

- Trimming Knob (3) located at left side of the machine. Press it to middle position, trimming thickness: 15 μ m. Press it to bottom, trimming


thickness is 30 μ m

- Firstly, move the blade holder base close to Specimen but do not touch it.

Then fasten the blade holder to make trimming and sectioning.

- Or Press knob (1) to choose big value range, for example(50 μ m) to make trimming

- When specimen at upper position, press the trimming knob to make trimming, likewise until the surface

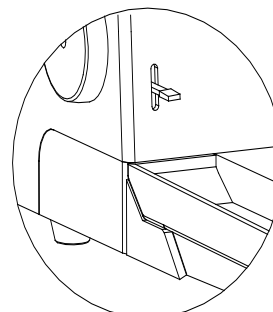

of specimen suitable to make sectioning

8.4 Sectioning

Attention: Be sure to turn the handwheel evenly and the speed of handwheel turning should match the rigidity of the specimen. The harder, the slower.

Section thickness value achieved by adjusting section knob at right upright of the machine.

- Choose best cutting angle, from small to big scale. Once the specimen is too hard to cut,

Cutting angle should be big

- Scale Value at right side of the blade holder is

Used to adjust cutting angle


- Rotate Section Handwheel smoothly and

Evenly to get ideal, good sample

8.5 Retraction

- Button of retraction function located back of the Machine, Button "ON" and Button "OFF"

- Use "Single" Screwdriver to turn the button to "ON", it means retraction function is used, if turn to "OFF", it means retraction function is shut off

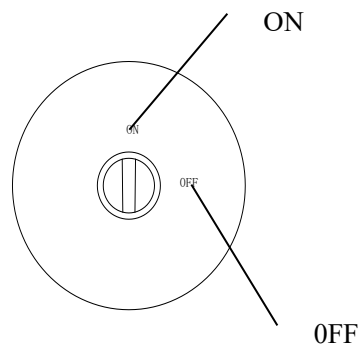

9. Regular Operation

Instruction to the procedure of paraffin Sectioning

Attention: Be sure to lock the handwheel and cover the edge of the blade with the blade protecting fitting in the course of operating of the blade and specimen or before changing the specimen.

- Lock the handwheel

Attention: Firmly clamp the specimen before installing the blade.

- Put the pre-frozen paraffin onto the specimen clamp.

Attention: Be sure to be careful enough to avoid misoperation which will cause serious hurt in the course of using the blade and disposable blade, because the edge of the blade is very sharp.

- Turn the handwheel to move the specimen to the backward utmost position.
- Insert the blade into the blade holder and firmly clamp it.
- Adjust the cutting angle (try once from 0° to 3°)



- Try to move the blade holder approaching the specimen.
- Adjust the surface position of the specimen to make it parallel to the edge of the blade.
- Loosen the handwheel.

Attention: Be sure to turn the handwheel evenly in the course of the slice cutting. The harder, the slower.

- Turn the handwheel to start the slice-trimming for the ideal surface of the specimen.
- Select the ideal thickness of the slice or take the former ones as reference.
- Evenly turn the handwheel clockwise to cut slice.
- Change the specimen or stop the operation.

Attention: Be sure to lock the handwheel and cover the edge of the blade with the blade protecting fitting in the course of operating of the blade and specimen or before changing the specimen or during the break.

- Lock the handwheel.
- Cover the edge of the blade with the blade protecting fitting.
- Take out the specimen from the specimen-clamp for another operation.

End the operation

- Lock the handwheel.
- Take out the blade from the holder and put it into the blade-case.
- Take out the specimen from the specimen-clamp.
- Scrub away the wastes and clean up the instrument.

10. Error Checking and Solution

Faults	Causes	Eliminations
Uneven slices produced and sometimes no slice can be cut	<ol style="list-style-type: none"> 1. Inappropriate angle of the blade, the angle of cutting is too small 2. Not firmly locked the specimen clamp or/and the blade holder. 3. Blunt of the blade 	<ol style="list-style-type: none"> 1. Adjust the angle of cutting until the appropriate angle acquired. 2. Check and firmly locked the screw of the specimen locking and the blade holder. 3. Use the other section of the blade or change for a new one.
Slices are compressed or corrugated or extruded	<ol style="list-style-type: none"> 1. Blunt of the blade. 2. The specimen is too hot. 3. The angle of cutting is too big. 4. The cutting is too fast. 	<ol style="list-style-type: none"> 1. Use the other section of the blade or change for a new one. 2. Freeze the specimen on the freezing platform. 3. Adjust the cutting angle. 4. Turn the handwheel slowly.

When cutting hard specimen, the blade holders; nicks or vibrant marks are left on the slice	1. The cutting is too fast. 2. The angle of cutting is too big. 3. Not firmly locked the specimen clamp or/and the blade holder.	1. Turn the handwheel slowly. 2 Adjust the cutting angle. 3. Check and firmly locked the screw of the specimen locking and the blade holder or the locking handle.
---	--	--

11. Cleaning

Attention: Be sure to lock the handwheel before cleaning

Brush off the slice crumbs with a dry brush.

Take down the blade basal and the blade holder for cleaning.

Attention: ◆ Only the cleanser for domestic use or the soap lye can be used for cleaning the instrument.

◆ Acetone and benzene will damage the paint on the surface of the instrument.


◆ No leakage of the cleaning liquid allowed into the instrument.

◆ A moist cloth is needed for the cleaning.

12. Maintenance

Generally, the microtome can work normally for a long time without any maintenance. But the preventive maintenance is also needed to ensure that the instrument can work normally in a longer period. The regular maintenance should follow the advice listed below:

- Have the technician authorized by our company check the instrument at least once a year.
- After the free service period a successive maintenance contract should be made to ensure the service. The detail can be consulted with the Kalstein service agencies.
- Clean the microtome daily.
- Monthly lubricate the following parts with the oil we offered (one or two drop is enough):
 - ① The “T” block (1) on the base of the instrument.
 - ② the guiding rod (2) of the basal of the blade holder on the base of the instrument.

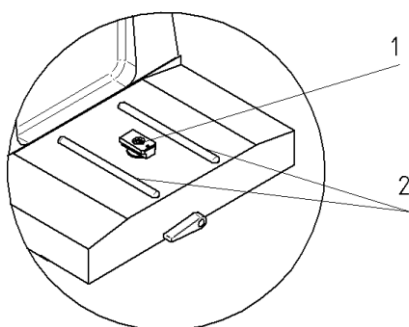

- The maintenance should be done by the authorized technicians. And no self-repair is allowed, or we will not be responsible for the result of self-repair and further maintenance.

13. Appendix

Improvement of the instrument

Our company has the right to change the technical parameters of any Model for improving the function of the instruments. Excuse us for not informing the customers in advance.



Quality guarantee

It is for sure that every instrument we sell has been strictly examined to ensure that every instrument is qualified and matches its technical standard.

The free service terms which are favorable to the customers are made for the sales agencies.

Free service terms are only provided for those who regularly use of the instrument and operate the instrument according to the Instructions.

We will not be responsible for the damage and other results caused by abuse and misoperation of the instrument.

Discards and disposition

The discarded microtome and its fittings should be disposed according to the current laws or regulations.

For the sake of environmental protection, we are willing to give you some advice on discarding YR417 microtome.

Service information for customers

If you need any service or fittings of the instrument in the guaranteed usable period, please consult the agencies of our company or the sellers. But you should provide them the specification, model, the serial number and the time of the buying.

Attention:

If you mail the instrument or its fittings back to Kalstein France company, please make sure the following:

- If the instrument or its fittings has handled the substance with virus and bacteria or contacted with radiation resources, please disinfect them or eliminate the radioactivity before mailing back. Our technicians will examine and verify for sure.
- If you are sure that the instrument or its fittings you want to send back to our company is safe from infection of virus, bacterium or radiation, please tell our technician the possible ways you will use to disinfect them or eliminate the radioactivity. Any possible infection of dangerous bacterium and virus or radiation will lead to sending back the instrument or its fittings without any maintenance.

For technical service, please inform us:

- The type and the serial number of the instrument
- Address and the person for contacting
- The causes for the service.



All rights reserved © KALSTEIN France S. A. S.,
2 Rue Jean Lantier • 75001 Paris •
+33 1 78 95 87 89 / +33 6 80 76 07 10 •
<https://kalstein.eu>
KALSTEIN FRANCE, S. A. S

